


Valar Peptides

Certificate of Analysis (CoA)

Product:	BPC-157 Capsules
Quantity:	500 mcg
Batch/Lot No.:	BPCU500-03-816-e382
Date of Analysis:	17 Nov 2025
Instrument:	Agilent 1260 HPLC and Thermo (MK3)

Quality Control

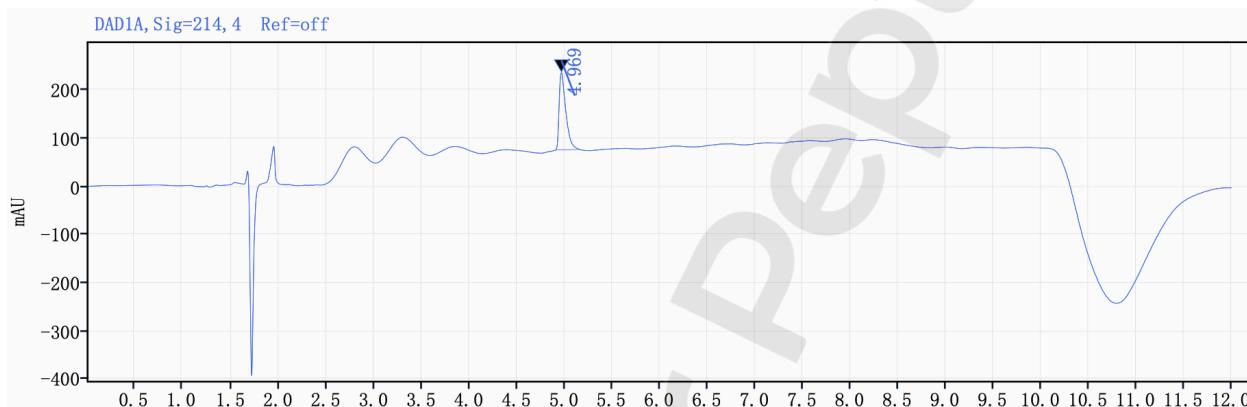

Test Parameter	Method	Specification	Result
Identification (Retention Time)	Visual inspection	White to off-white lyophilized powder (conforms)	White to off-white lyophilized powder (conforms)
Identification (Retention Time)	HPLC	± 0.2 min of Standard	Conforms
Purity (by HPLC, % area)	HPLC	$\geq 99.0\%$	99.91%
Net Peptide Quantity	HPLC	500mcg	480 mcg
Endotoxin	LAL	≤ 0.5 EU/mg	Conforms

Authorized by:

Matt C.

Head of Quality Control