


# Valar Peptides

## Certificate of Analysis (CoA)

<b>Product:</b>	GHK-Cu
<b>Quantity:</b>	50mg
<b>Batch/Lot No.:</b>	GK50-01-905-g387
<b>Date of Analysis:</b>	20 Nov 2025
<b>Instrument:</b>	Agilent 1260 HPLC and Thermo (MK3)

### Quality Control

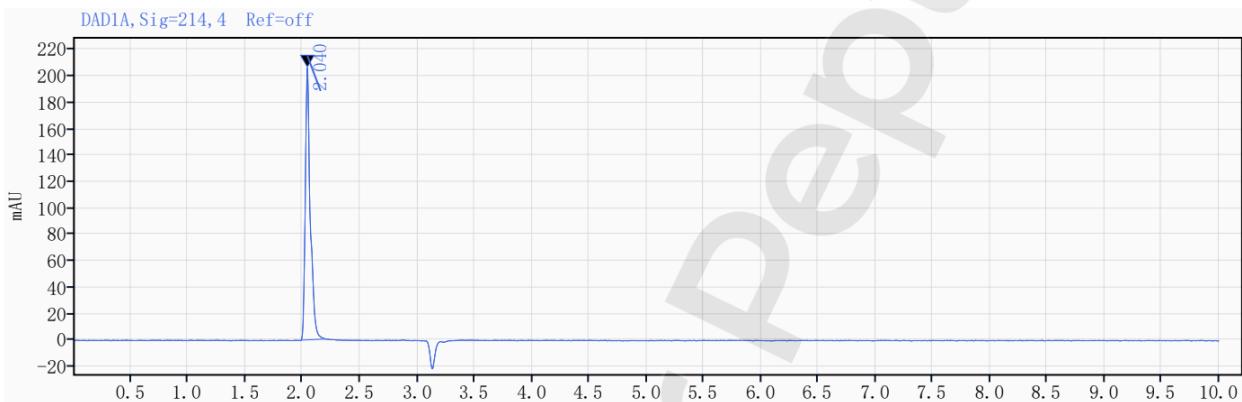

Test Parameter	Method	Specification	Result
Identification (Retention Time)	Visual inspection	Blue to off-blue lyophilized powder	Blue to off-blue lyophilized powder (conforms)
Identification (Retention Time)	HPLC	$\pm 0.2$ min of Standard	Conforms
Purity (by HPLC, % area)	HPLC	$\geq 99.0\%$	99.88%
Net Peptide Quantity	HPLC	50mg	52.27 mg
Endotoxin	LAL	$\leq 0.5$ EU/mg	Conforms

Authorized by:

Matt C.

Head of Quality Control