


# Valar Peptides

## Certificate of Analysis (CoA)

<b>Product:</b>	BPC157, TB500 and GHK-Cu (Glow)
<b>Quantity:</b>	5mg / 5mg / 20mg
<b>Batch/Lot No.:</b>	GL05-03-814-f470
<b>Date of Analysis:</b>	28 Nov 2025
<b>Instrument:</b>	Agilent 1260 HPLC and Thermo (MK3)

### Quality Control

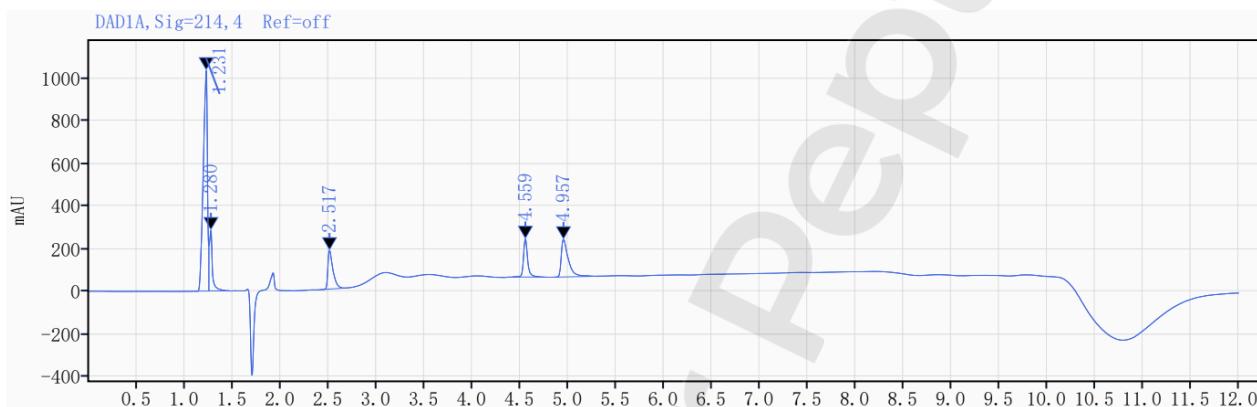

Test Parameter	Method	Specification	Result
<b>Identification (Retention Time)</b>	Visual inspection	Blue to off-Blue lyophilized powder	Blue to off-Blue lyophilized powder (conforms)
<b>Identification (Retention Time)</b>	HPLC	$\pm 0.2$ min of Standard	Conforms
<b>Purity (by HPLC, % area)</b>	HPLC	$\geq 99.0\%$	99.05%
<b>Net Peptide Quantity</b>	HPLC	5mg / 5mg / 20mg	5.07mg / 5.01mg / 19.41mg
<b>Endotoxin</b>	LAL	$\leq 0.5$ EU/mg	Conforms

Authorized by: Matt C.  
Matt C.  
Head of Quality Control