


Valar Peptides

Certificate of Analysis (CoA)

Product:	BPC157, TB500 and GHK-Cu (Glow)
Quantity:	10mg / 10mg / 65mg
Batch/Lot No.:	GL10-03-1017-g468
Date of Analysis:	21 Oct 2025
Instrument:	Agilent 1260 HPLC and Thermo (MK3)

Quality Control

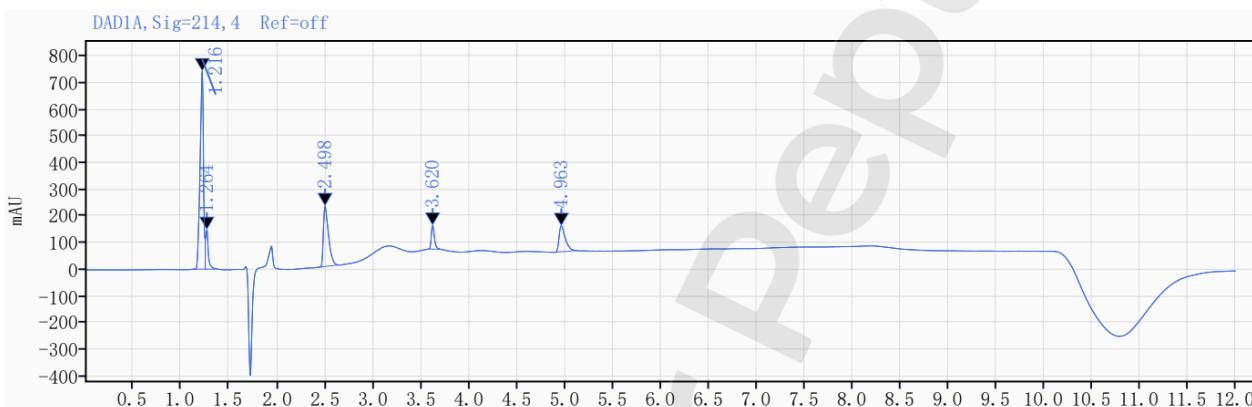

Test Parameter	Method	Specification	Result
Identification (Retention Time)	Visual inspection	Blue to off-Blue lyophilized powder	Blue to off-blue lyophilized powder (conforms)
Identification (Retention Time)	HPLC	± 0.2 min of Standard	Conforms
Purity (by HPLC, % area)	HPLC	$\geq 99.0\%$	99.02%
Net Peptide Quantity	HPLC	10mg / 10mg / 65mg	10.22mg / 11.82mg / 65.37mg
Endotoxin	LAL	≤ 0.5 EU/mg	Conforms

Authorized by: 
Matt C.
Head of Quality Control